

Fig.1

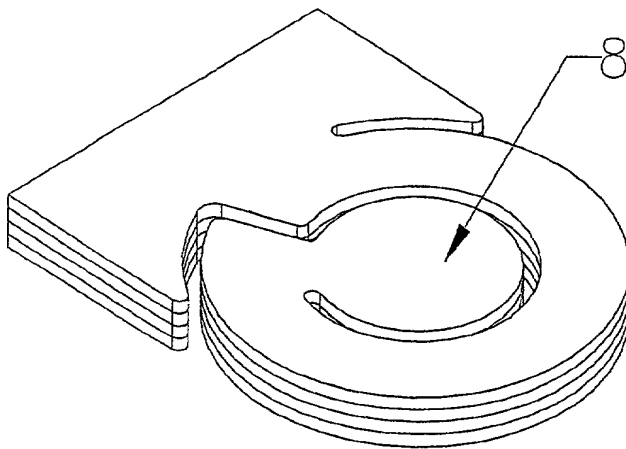


Fig.2

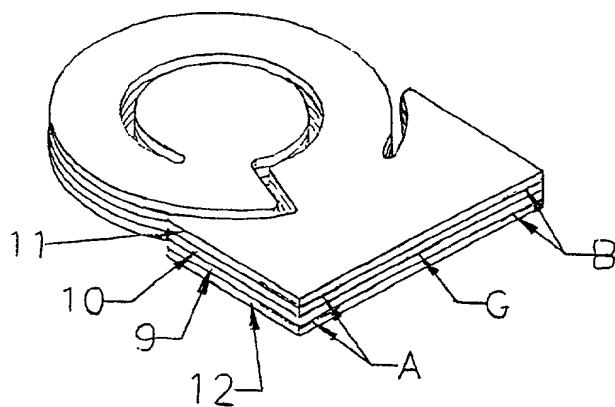


Fig.3

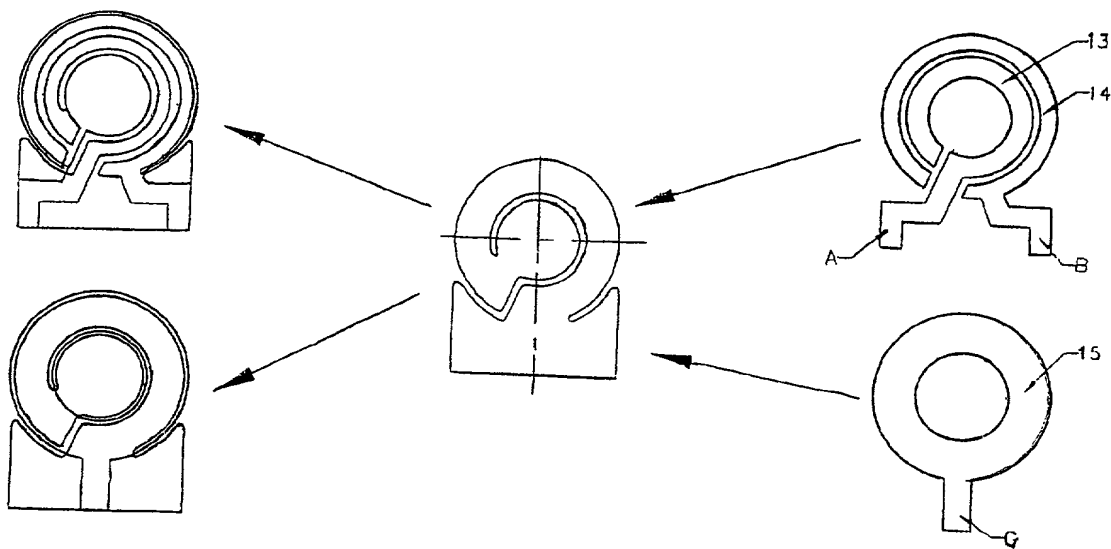


Fig.4

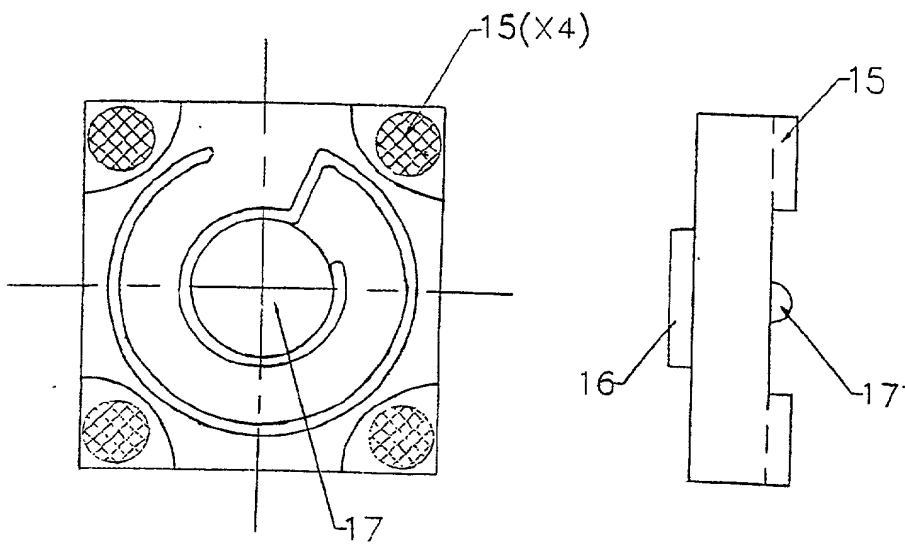


Fig.5

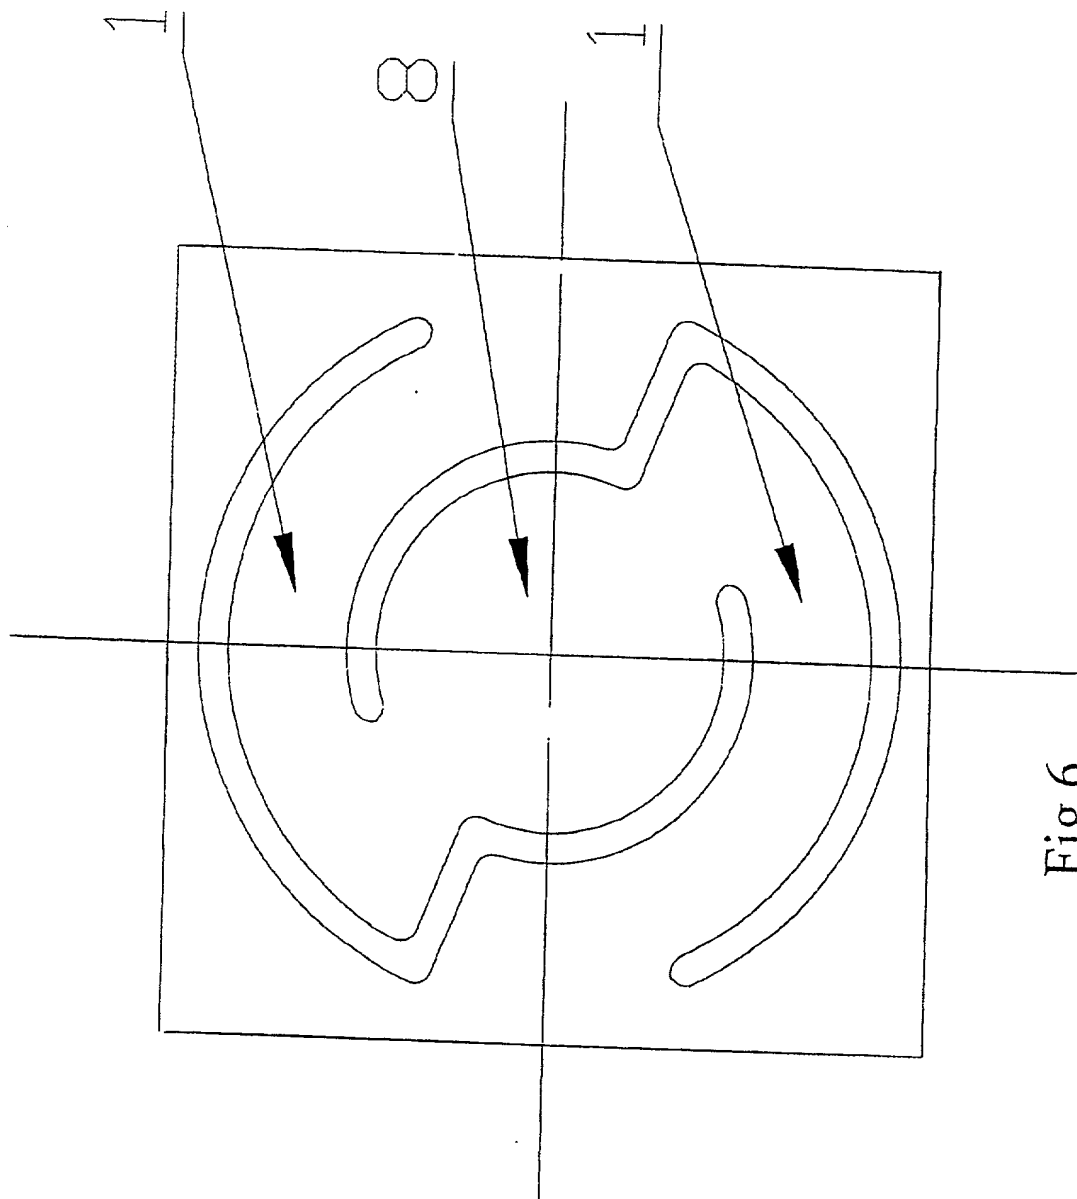


Fig.6

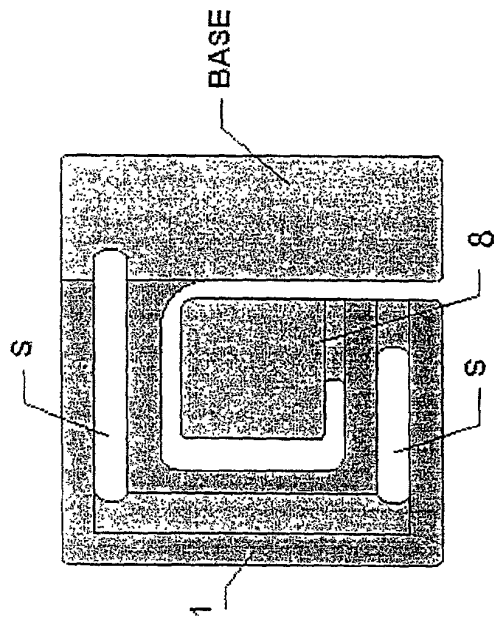


Fig.7

FIG. 7 is a cross-sectional view of the device of FIG. 6, showing the device in a closed position. The device is shown in a cross-sectional view, with the base 1 and the top 2. The device is shown in a closed position, with the top 2 being in contact with the base 1. The device is shown in a cross-sectional view, with the base 1 and the top 2. The device is shown in a closed position, with the top 2 being in contact with the base 1.

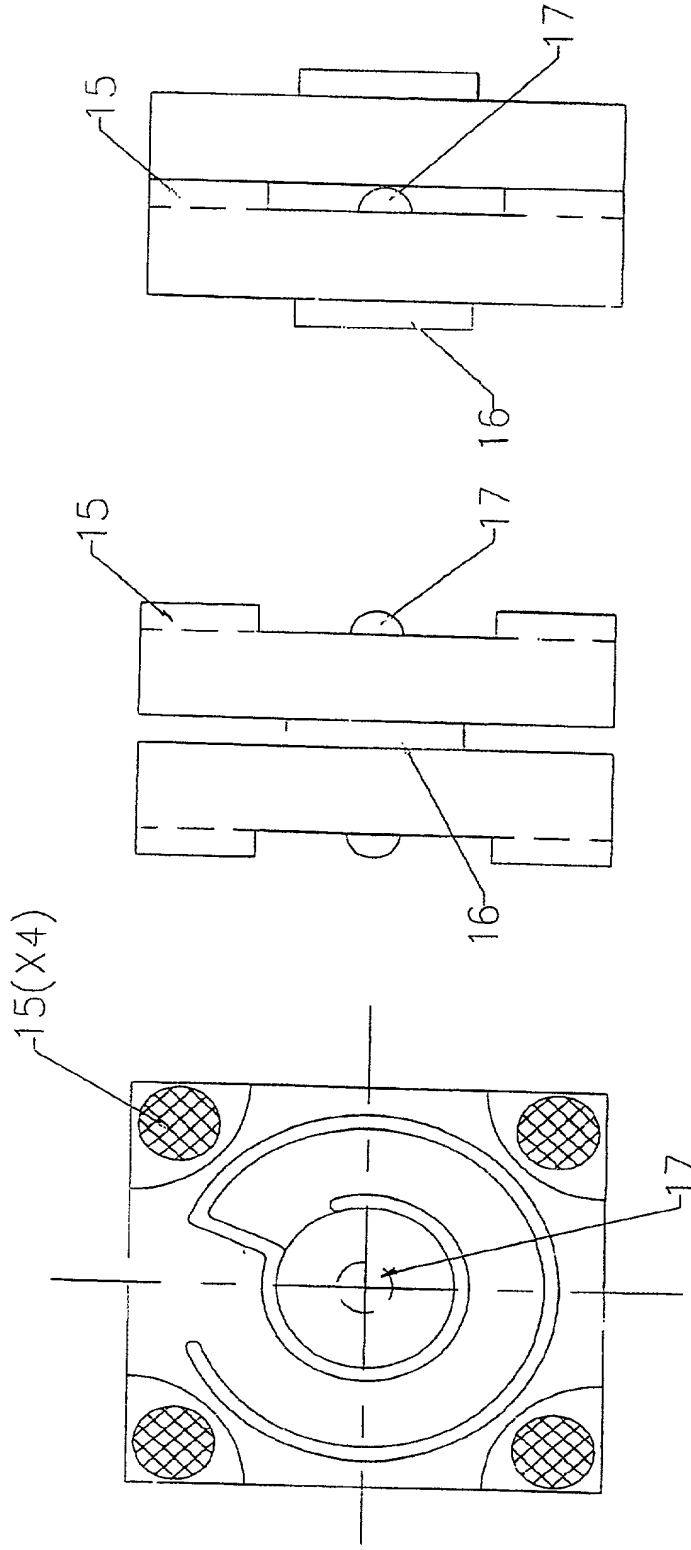


Fig.8

Fig.8A

Fig.8B

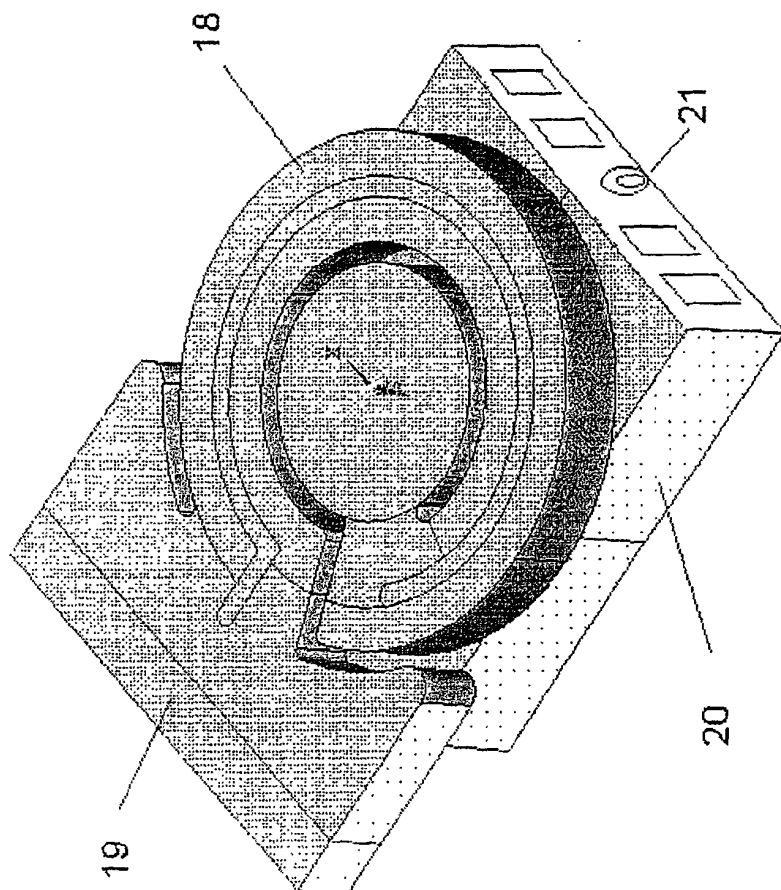


Fig.9

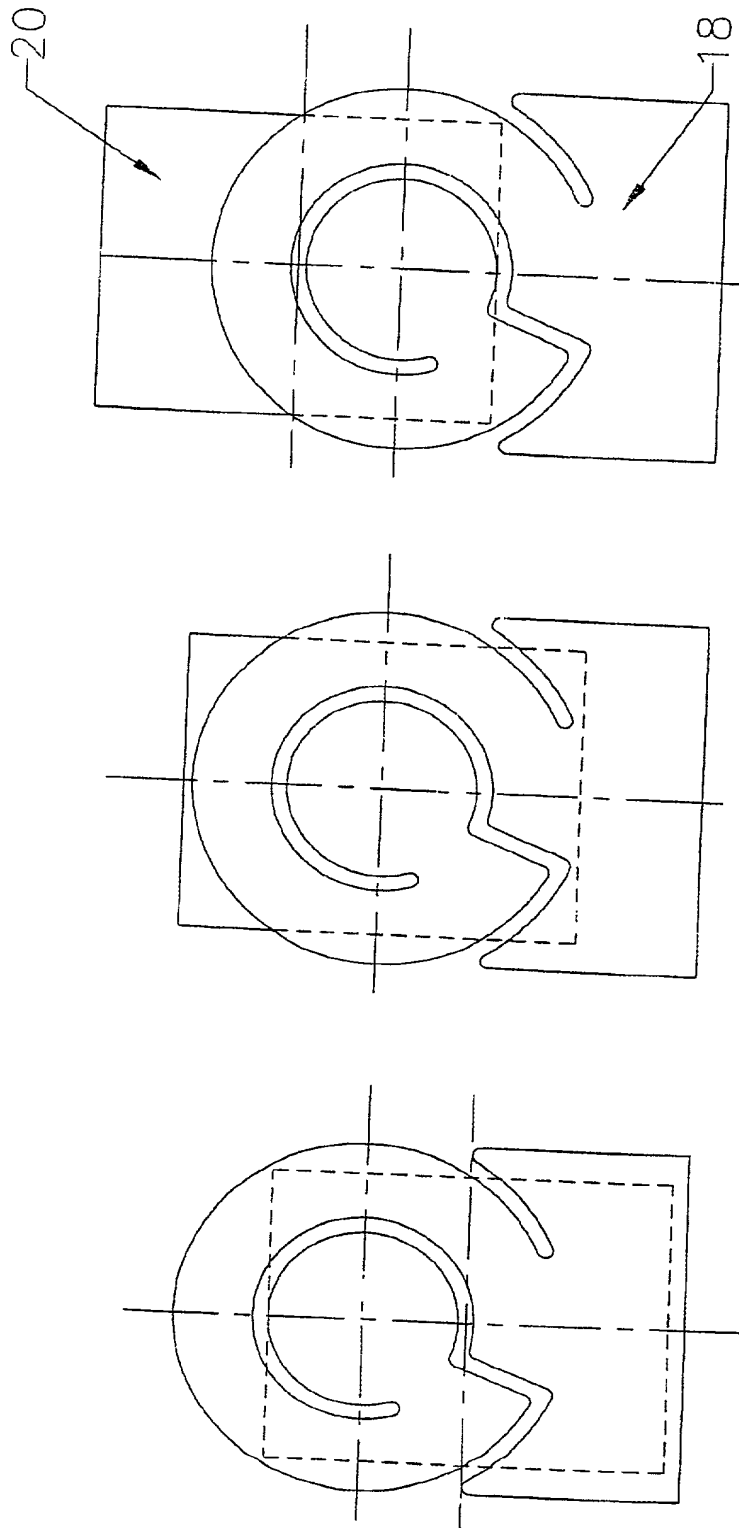


Fig.10



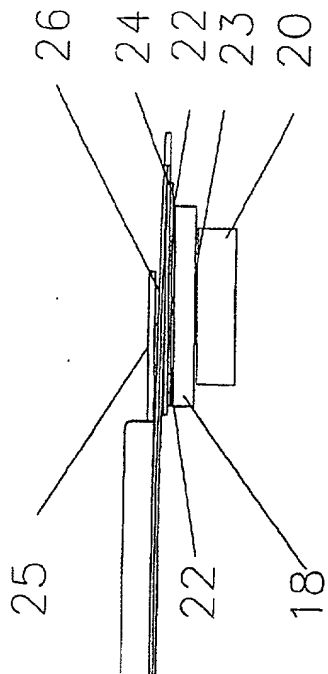


Fig.11

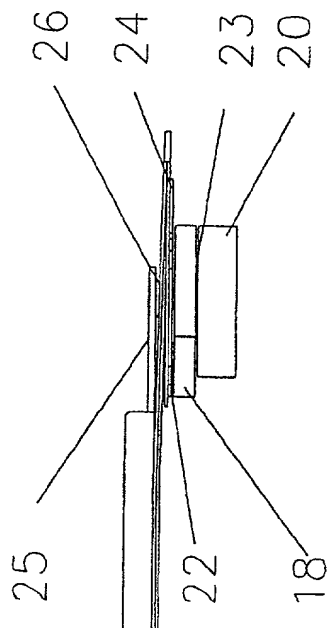


Fig.12

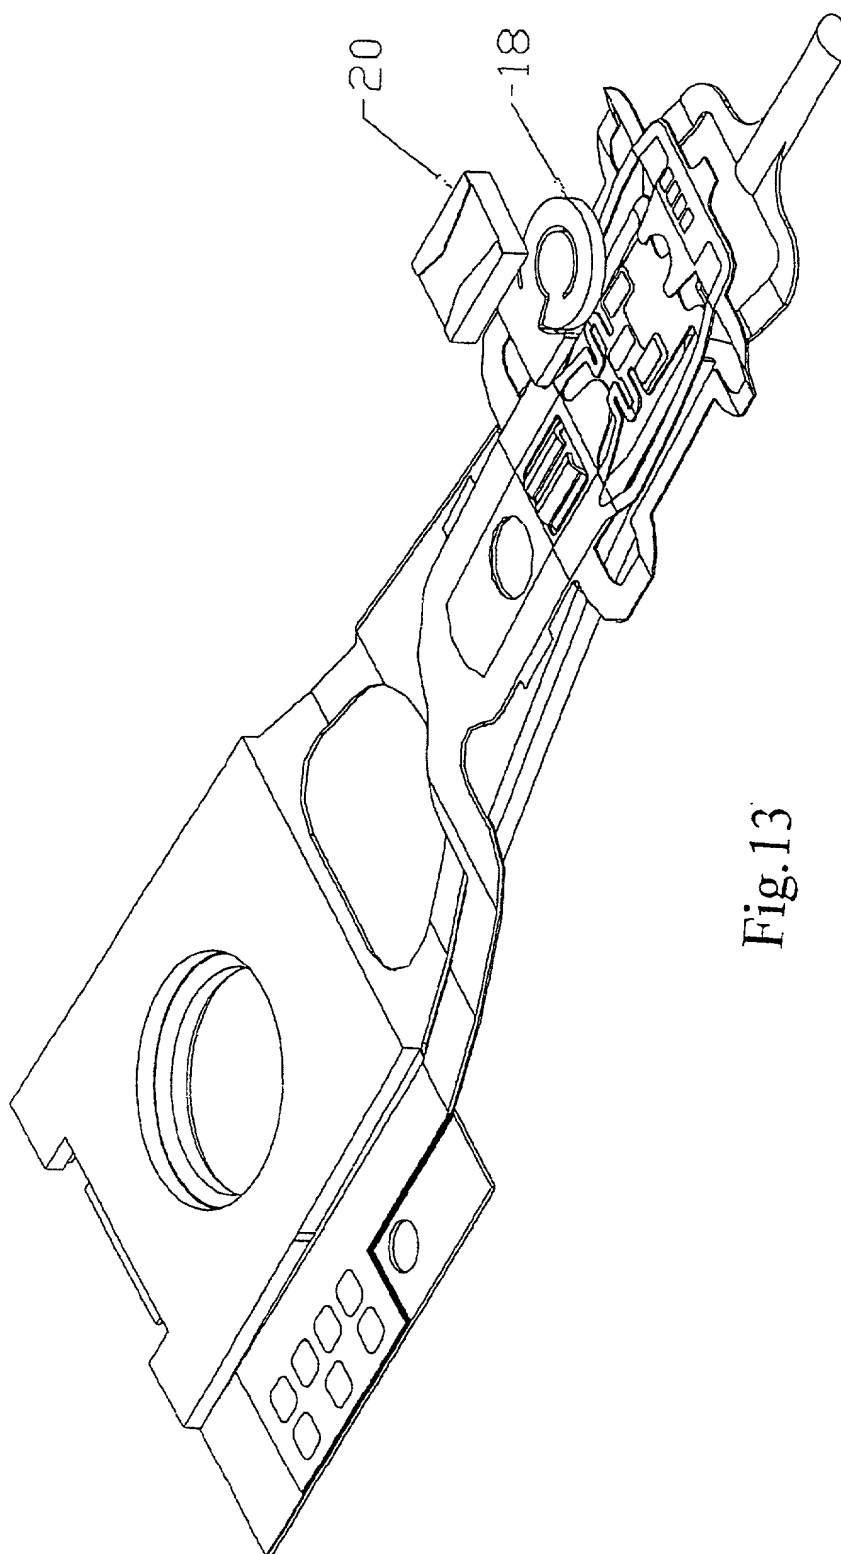


Fig. 13